


REFILL PACKAGE INSTRUCTIONS

How to easily refill Theraline micro-beads pillows:

Dear customers,

since April 2015 we decided to change the refill-opening of our pillows from zipper to an approximately 15 cm long and self-sealing tunnel opening. It might appear complicated in the beginning but we hope to have improved the refilling process for you. If at all only a few beads will fall to the ground or stick to your hands and clothes.


Your Theraline Team

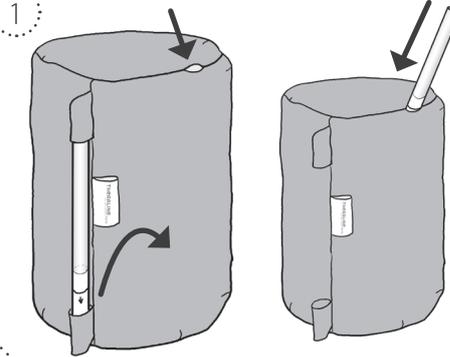

To refill a Theraline nursing pillow via the new refill-opening please proceed as follows:


You can easily handle it on your own but we recommend doing it in pairs. Choose a location for your refill where you can easily remove possibly leaking micro-beads with a vacuum cleaner. Take the tube out of the attachment and insert it into the opening at the seam of the refill package. Please make sure you only insert the tube until the marking.

2

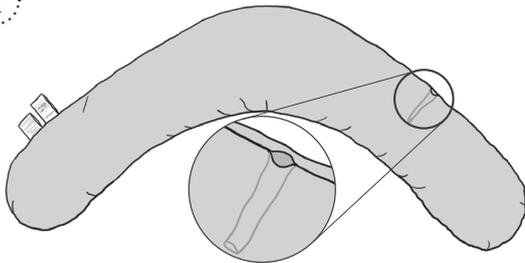

You can find the refill opening of the nursing pillow-inlet opposite to the care labels at the outer seam.

3

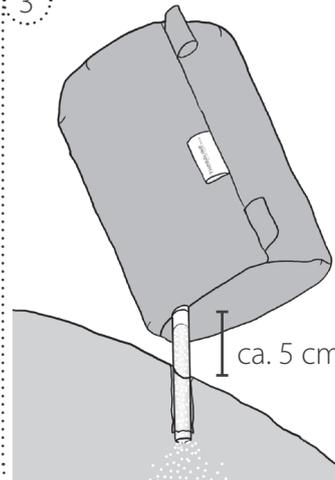

Hold the refill package with the tube facing up and insert the tube until approximately 5 cm into the refill opening of the inlet (meaning approx. 14 cm of the tube has to be inserted into the inlet). If the tube is not inserted deeply enough you will possibly not be able to refill the inlet. Now hold up the refill package for making the micro-beads flow into the inlet.

With the inlet being properly refilled please carefully pull the tube out. Beforehand make sure the tube is not still filled with micro-beads by letting them flow off to either the inlet or the refill package.

← into refill package ca. 5 cm | Viewing degree ca. 5 cm | Inlet ca. 14 cm →



THERALINE
love care comfort

Theraline eK
Industriepark Nord 56
D-53567 Buchholz Ww.

Tel: 026 83 - 96 96 0
Mail: info@theraline.de